SMD

www.smd-medical.com

Nasopharyngeal Airway

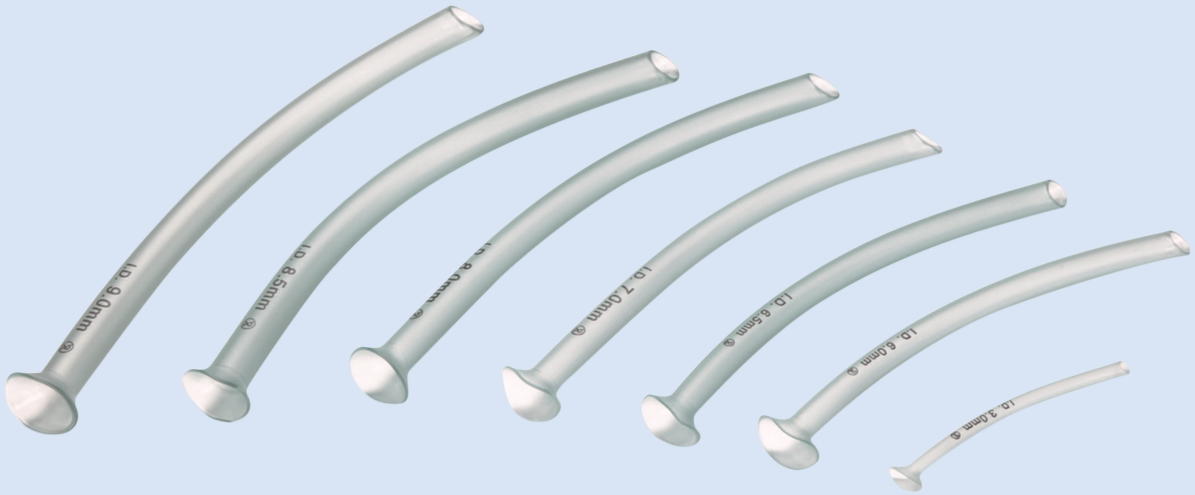

Instructions For Use:

- Designed to be inserted into the nasal passageway to secure an open airway.
- The correctly sized airway should be selected by measuring from the tip of the patient's nose to the bottom of their ear (angle of the jaw) and the diameter should be slightly smaller than the patient's nostril.
- Use universal precautions (eye protection, mask, gloves, etc.).
- Check for obstructions or fractures to the nose.
- Lubricate the device with a water-soluble gel, being careful not to block the tip.
- With the bevel tip directed toward the nasal septum, insert the airway. If resistance is felt, remove the airway and attempt in the other nostril.
- Insert until the flange is resting against the nostril opening.

Features:

- Material: medical grade, non-toxic PVC.
- For nasal airway management only.
- Atraumatic soft rounded beveled tip.
- Size: 2.5, 3.0, 3.5, 4.0, 4.5, 5.0, 5.5, 6.0, 6.5, 7.0, 7.5, 8.0, 8.5, 9.0, 9.5
- Green semi-transparent, blue semi-transparent or white semi-transparent.

Size	Ref	Material
2.5mm (10Fr)	236-2.5-12A	PVC
3.0mm (12Fr)	236-3.0-12A	PVC
3.5mm (14Fr)	236-3.5-12A	PVC
4.0mm (16Fr)	236-4.0-12A	PVC
4.5mm (18Fr)	236-4.5-12A	PVC
5.0mm (20Fr)	236-5.0-12A	PVC
5.5mm (22Fr)	236-5.5-12A	PVC
6.0mm (24Fr)	236-6.0-12A	PVC
6.5mm (26Fr)	236-6.5-12A	PVC
7.0mm (28Fr)	236-7.0-12A	PVC
7.5mm (30Fr)	236-7.5-12A	PVC
8.0mm (32Fr)	236-8.0-12A	PVC
8.5mm (34Fr)	236-8.5-12A	PVC
9.0mm (36Fr)	236-9.0-12A	PVC
9.5mm (38Fr)	236-9.5-12A	PVC

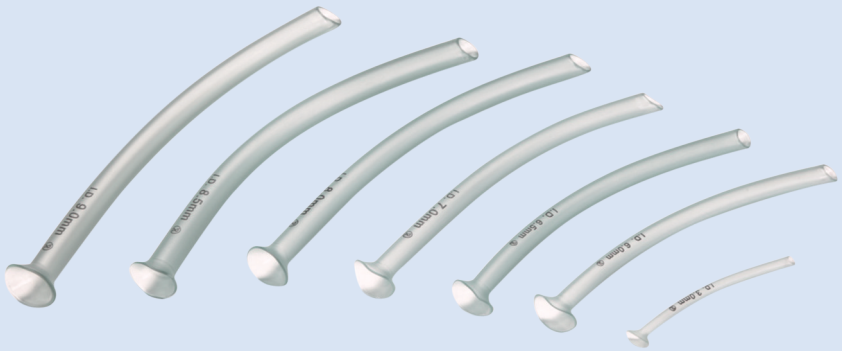

Contraindications:

1. Nasal infection.
2. Nasal deformity.
3. Abnormal anticoagulant mechanism.
4. Should never be used in patients with severe head or facial injuries, or have a suspected basilar skull fracture, as the tube can unintentionally enter into the brain tissue.

Caution:

1. Read instruction for use before using the device.
2. This product is sterilized for single use only, discard after single use. Please do not repeat sterilization, do not clean, do not use it once again.
3. Should be used the product immediately after opening the individual package, please destroy when it was used.
4. Do not use it if the inner package has been previously opened or damaged, or package be affected with damp, or the product went moldy.
5. Do not use after expiry date. If over the expiry date, please discard it.
6. Sterile by ETO. Single use only. Latex free.

Storage:

Store in a cool, dry and dark place. Avoid direct sunlight.

Nasopharyngeal Airway

SMD

www.smd-medical.com

Secured Medical Direction UK Co., Ltd.
Beautiful Group Tower 77 Connaught Road, Central, HK P.R.C.
EC REP MedPath GmbH
Mies-van-der-Rohe-Strasse 8, 80807 Munich, Germany

www.smd-medical.com