SMD
www.smd-medical.com

# Silicone Laryngeal Mask Airway

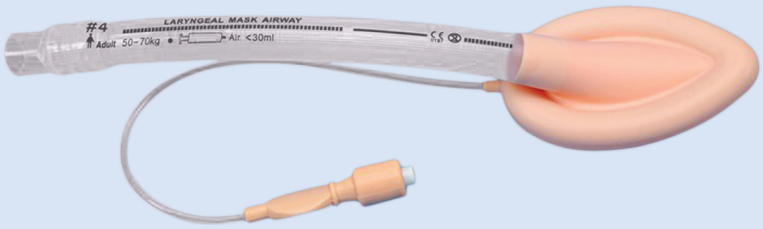

## Instructions For Use:

- Deflate the cuff completely so that it forms smooth “spoon-shape”. Lubricate the posterior surface of the mask with water-soluble lubricant.
- Hold the laryngeal mask like a pen, with the index finger placed at the junction of the cuff and the tube.
- With the head extended and the neck flexed, carefully flatten the laryngeal mask tip against the hard palate.
- Use the index finger to push cranially, maintaining pressure on the tube with the finger. Advance the mask until definite resistance is felt at the base of the hypopharynx.
- Gently maintain cranial pressure with the non-dominant hand while removing the index finger.
- Without holding the tube, inflate the cuff with just enough air to obtain a seal (to a pressure of approximately 60cm H2O). See the instructions for appropriate volumes. Never over inflate the cuff.

## Features:

- Size: 1.0, 1.5, 2.0, 2.5, 3.0, 4.0, 5.0.
- Consists of airway tube, cuff, connector, inflation tube, valve, pilot balloon.
- Easier operation and time saving than endotracheal tube during intubation.
- Less pain and cough caused than endotracheal tube.

**Name of parts for Silicone Laryngeal Mask Airway**

| Silicone Laryngeal Mask Airway | | |
|---|---|---|
| **Item No.** | **Name** | **Material** |
| 1 | Cuff | Silicone |
| 2 | Airway tube | Silicone |
| 3 | Connector | PP |
| 4 | Inflation tube | Silicone |
| 5 | Pilot balloon | Silicone |
| 6 | Valve | ABS |

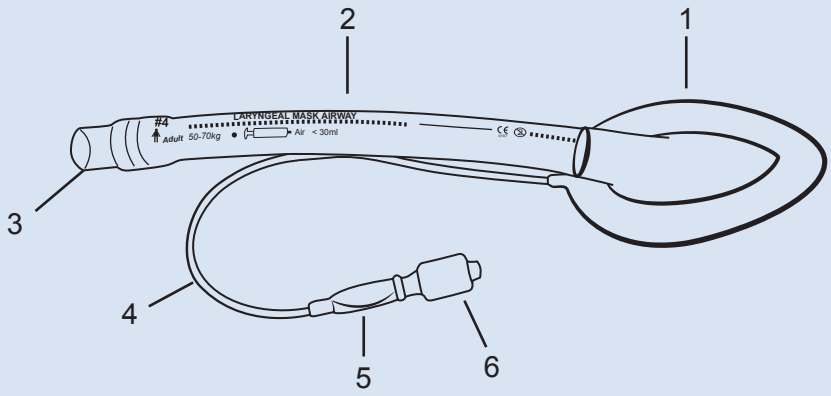


| Size | Patient Size | Max. Inflation Volume (ml) |
|---|---|---|
| 1.0 | Neonates up to 5 kg | 4 |
| 1.5 | Infants 5-10 kg | 7 |
| 2.0 | Infants/Children 10-20 kg | 10 |
| 2.5 | Children 20-30 kg | 14 |
| 3.0 | Children 30-50 kg | 20 |
| 4.0 | Adults 50-70 kg | 30 |
| 5.0 | Adults 70-100 kg | 40 |

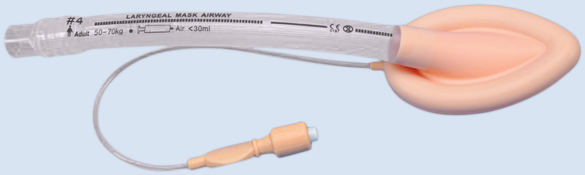

| Size | Ref |
|---|---|
| Silicone 1.0 | 20-1.0-12A |
| Silicone 1.5 | 20-1.5-12A |
| Silicone 2.0 | 20-2.0-12A |
| Silicone 2.5 | 20-2.5-12A |
| Silicone 3.0 | 20-3.0-12A |
| Silicone 4.0 | 20-4.0-12A |
| Silicone 5.0 | 20-5.0-12A |
| Silicone 1.0 | 20-1.0-12AB |
| Silicone 1.5 | 20-1.5-12AB |
| Silicone 2.0 | 20-2.0-12AB |
| Silicone 2.5 | 20-2.5-12AB |
| Silicone 3.0 | 20-3.0-12AB |
| Silicone 4.0 | 20-4.0-12AB |
| Silicone 5.0 | 20-5.0-12AB |

## Caution:

1. Read instruction for use before using the device.
2. This product is sterilized for single use only, discard after single use. Please do not repeat sterilization, do not clean, do not use it once again.
3. Should be used the product immediately after opening the individual package, please destroy when it was used.
4. Do not use it if the inner package has been previously opened or damaged, or package be affected with damp, or the product went moldy.
5. Do not use after expiry date. If over the expiry date, please discard it.
6. Do not exceed the recommended maximum inflation volumes.
7. Sterile by ETO. Single use only. Latex free.

## Storage:

Store in a cool, dry and dark place. Avoid direct sunlight.

# Silicone Laryngeal Mask Airway

SMD

www.smd-medical.com

**Secured Medical Direction UK Co., Ltd.**
Beautiful Group Tower 77 Connaught Road, Central, HK P.R.C.
EC REP MedPath GmbH
Mies-van-der-Rohe-Strasse 8, 80807 Munich, Germany

www.smd-medical.com